


363-U1484

U1484A, U1484B, U1484C

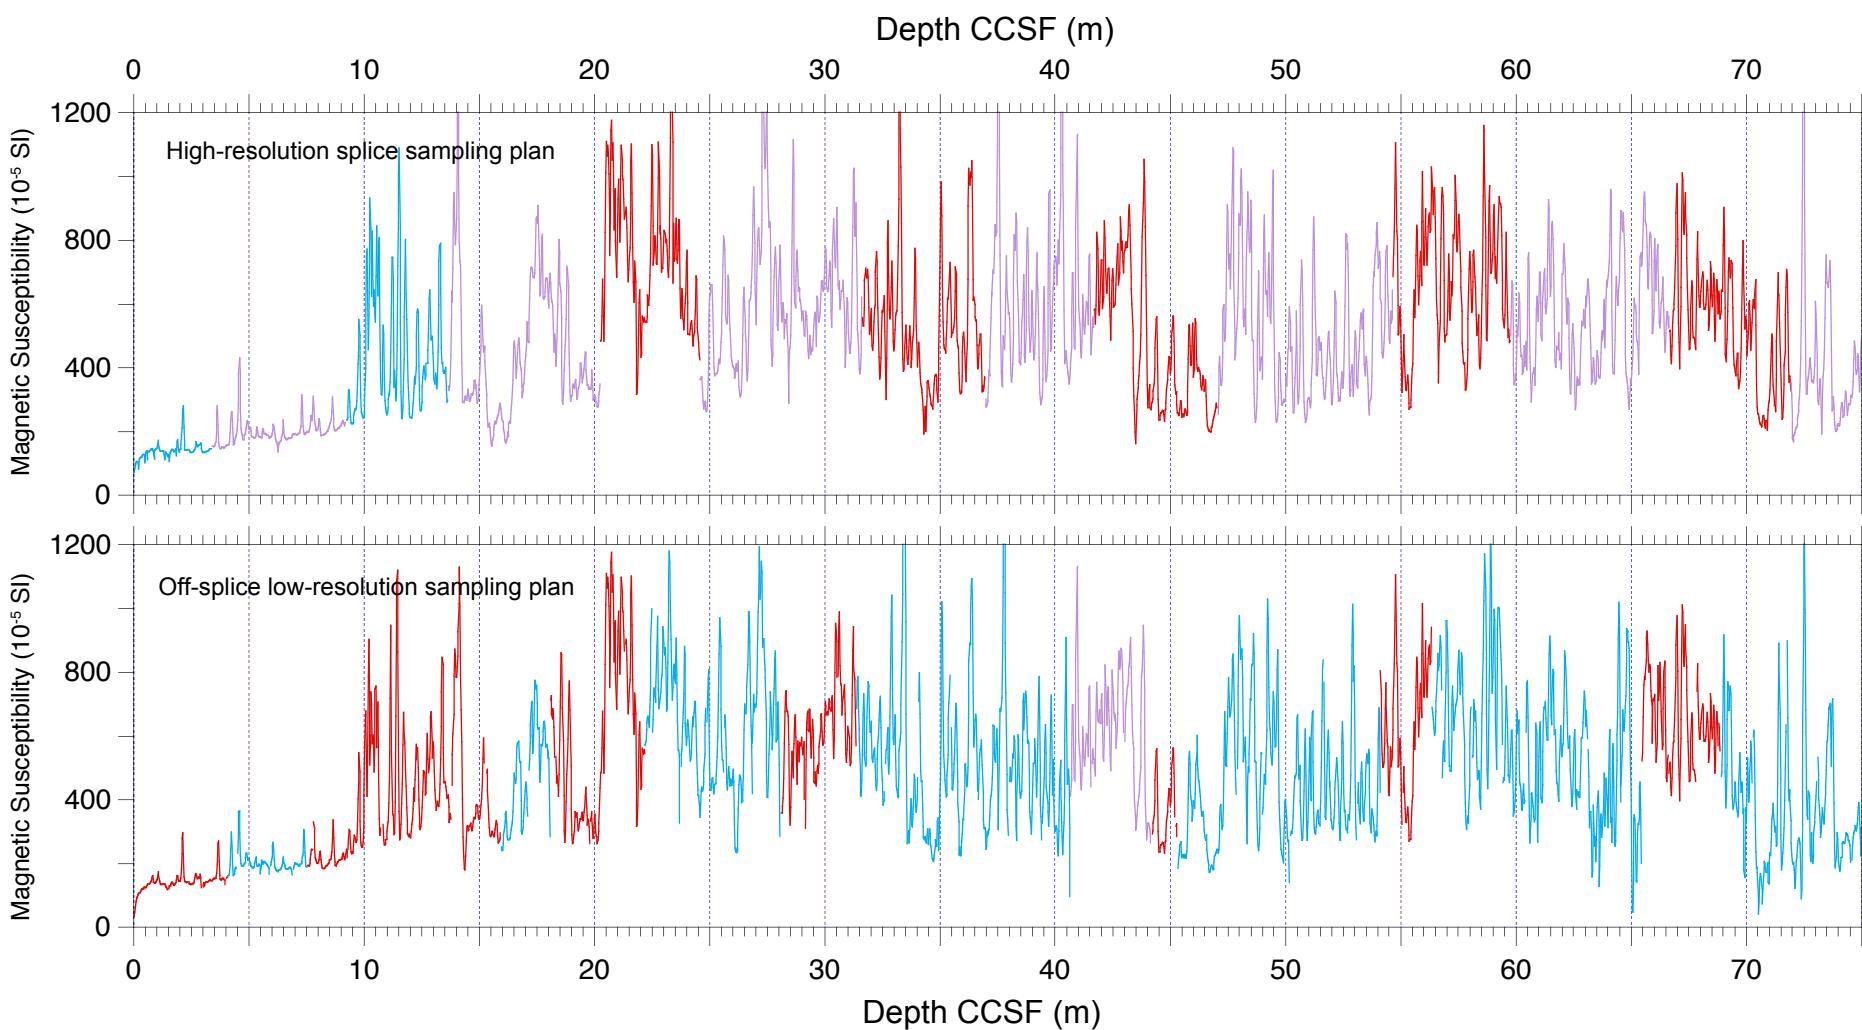


Supplementary Figure 3A-D. Comparison of magnetic susceptibility records at Site U1484 constructed using the high-resolution splice interval table (top panel) and the off-splice interval table for low-resolution sampling (bottom panel).

Expedition 363 Stratigraphic Correlation Off-splice Tables
Supplementary Figure 3B

363-U1484

U1484A, U1484B, U1484C


Depth CCSF (m)

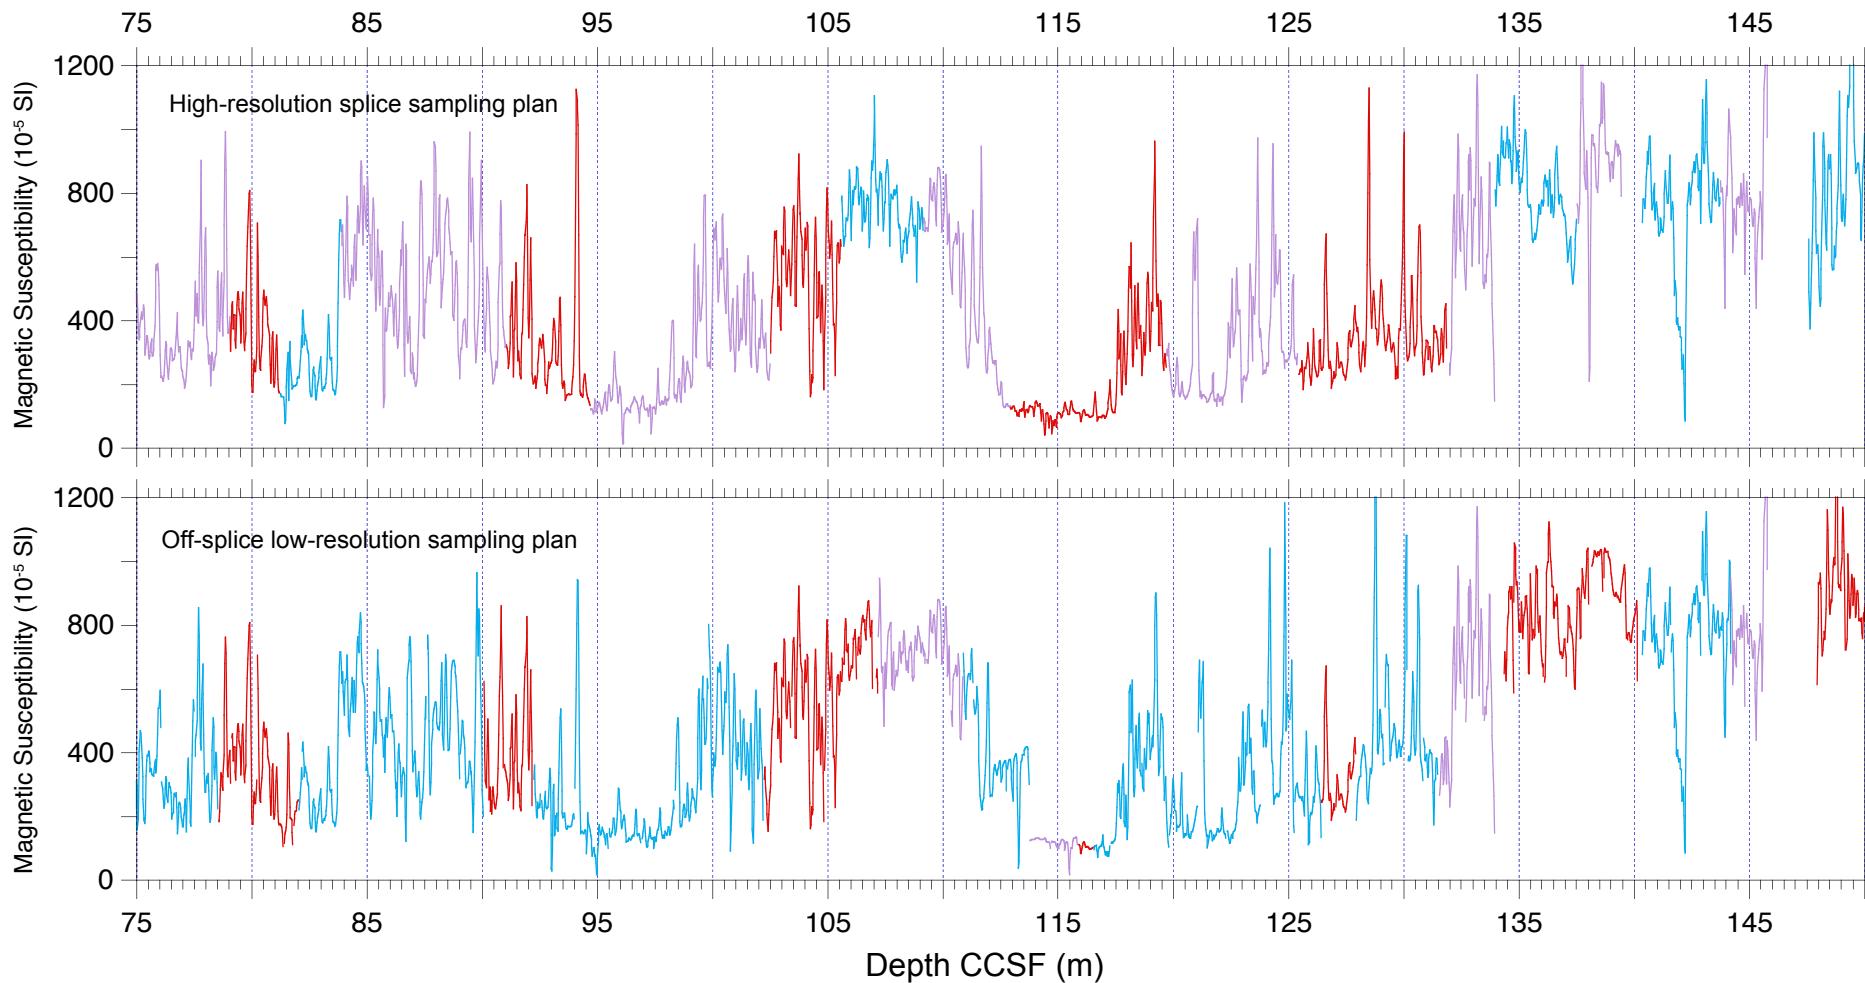

363-U1484

U1484A, U1484B, U1484C

Depth CCSF (m)

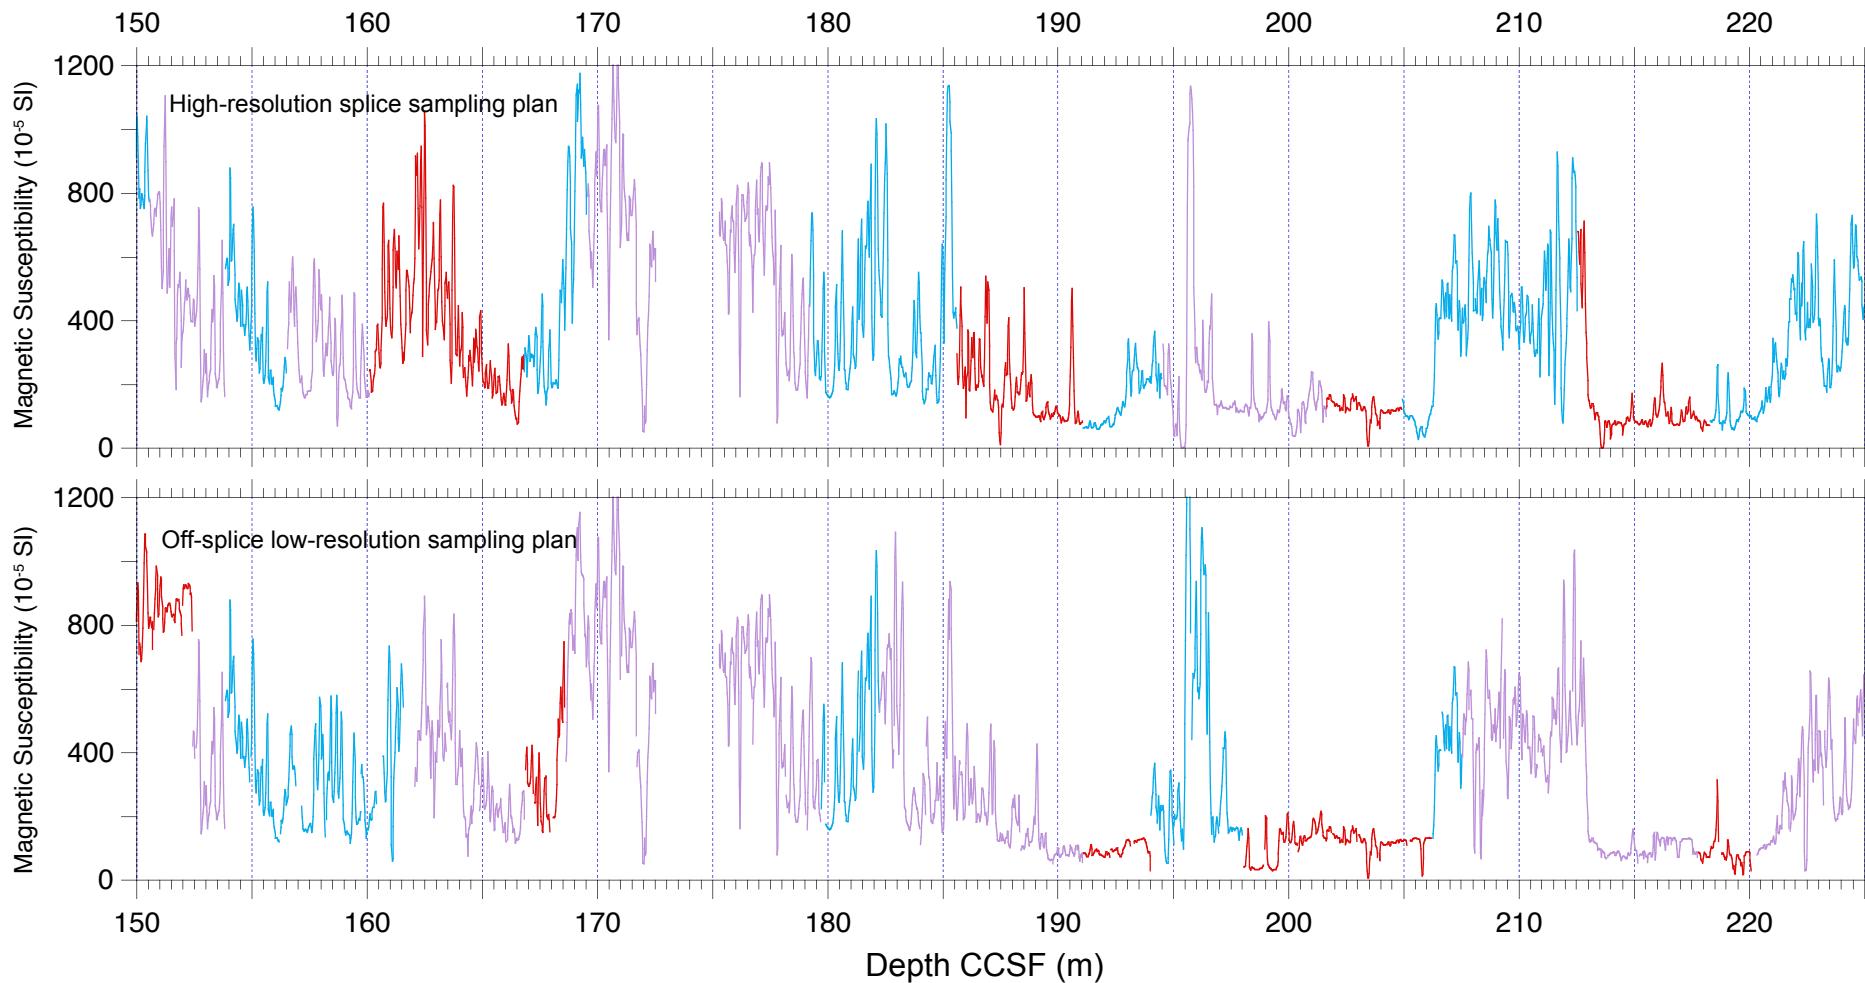

Expedition 363 Stratigraphic Correlation Off-splice Tables
Supplementary Figure 3D

363-U1484

U1484A, U1484B, U1484C

Depth CCSF (m)

